

CSUS

by Allard USA

C|s

PATELLA TRACKING SUPPORT

Rx Only — Single Patient Use Only

C|s

Instructions for Use



FEEL THE FUNCTION

The intended function of this brace is to provide gentle counter "traction" to the patella to help prevent the patella from shifting out of position. Review instructions on back page carefully before application.

For questions, please contact your physician, the professional who fit this device or Allard USA Customer Service:

CALL: 888-678-6548 FAX: 800-289-0809
info@allardusa.com

Allard USA, Inc. 300 Forge Way, Suite 3 Rockaway, NJ 07866-2056
www.allardusa.com

CSUS

by Allard USA

C|s

PATELLA TRACKING SUPPORT

Rx Only — Single Patient Use Only

C|s

Instructions for Use



FEEL THE FUNCTION


The intended function of this brace is to provide gentle counter "traction" to the patella to help prevent the patella from shifting out of position. Review instructions on back page carefully before application.

For questions, please contact your physician, the professional who fit this device or Allard USA Customer Service:


CALL: 888-678-6548 FAX: 800-289-0809
info@allardusa.com

Allard USA, Inc. 300 Forge Way, Suite 3 Rockaway, NJ 07866-2056
www.allardusa.com


Patella Tracking Support

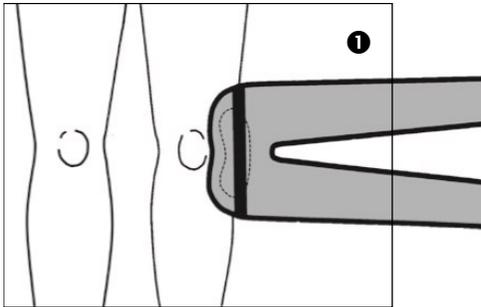

1. Depending on direction of instability, place the curved edge of the foam pad snugly against that side of the patella.

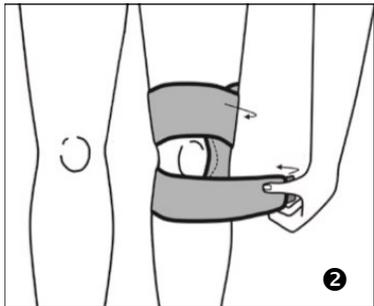

2. Wrap the upper wide strap above the patella, around the leg until comfortably snug and secure end. Repeat for the lower wide strap.

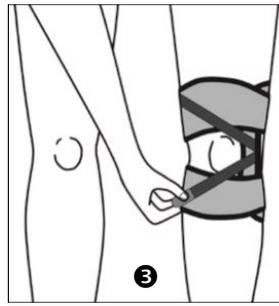

3. Pull the upper 1in strap upward and secure on the upper wide strap. Pull the lower 1in strap downward and secure on lower wide strap. Adjust 1 in straps as needed.

Indications / Intended Use

Medial or lateral patella instability, subluxation, chondromalacia, or misalignments of the patella, anterior knee pain.

Contraindications

Excessive edema when compression may impede circulation.

Adjustment

This brace should only be fitted by a licensed medical professional.

Warning

Do not overtighten, as this can cause poor circulation and/or skin irritation. If you feel any irritation, observe skin discoloration, or experience other problems such as excess swelling, remove support and consult your healthcare professional. Check skin on a daily basis.


Wash instruction

Hand wash in cold water using mild detergent. Air dry.


8716 Rev B

CSUS
by Allard USA


Patella Tracking Support

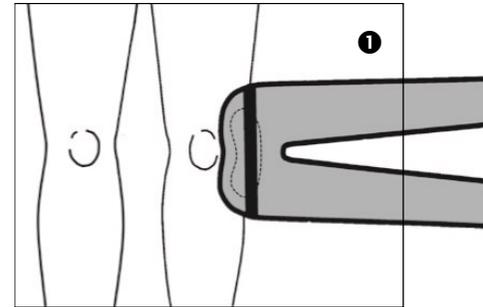

1. Depending on direction of instability, place the curved edge of the foam pad snugly against that side of the patella.

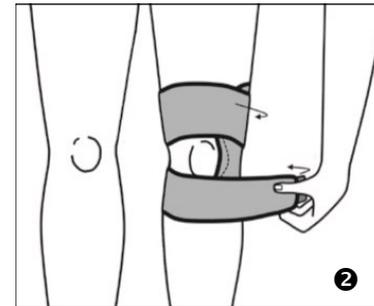

2. Wrap the upper wide strap above the patella, around the leg until comfortably snug and secure end. Repeat for the lower wide strap.

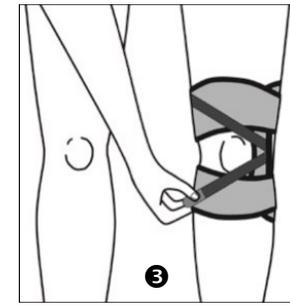

3. Pull the upper 1in strap upward and secure on the upper wide strap. Pull the lower 1in strap downward and secure on lower wide strap. Adjust 1 in straps as needed.

Indications / Intended Use

Medial or lateral patella instability, subluxation, chondromalacia, or misalignments of the patella, anterior knee pain.

Contraindications

Excessive edema when compression may impede circulation.

Adjustment

This brace should only be fitted by a licensed medical professional.

Warning

Do not overtighten, as this can cause poor circulation and/or skin irritation. If you feel any irritation, observe skin discoloration, or experience other problems such as excess swelling, remove support and consult your healthcare professional. Check skin on a daily basis.

Wash instruction

Hand wash in cold water using mild detergent. Air dry.

8716 Rev B

CSUS
by Allard USA